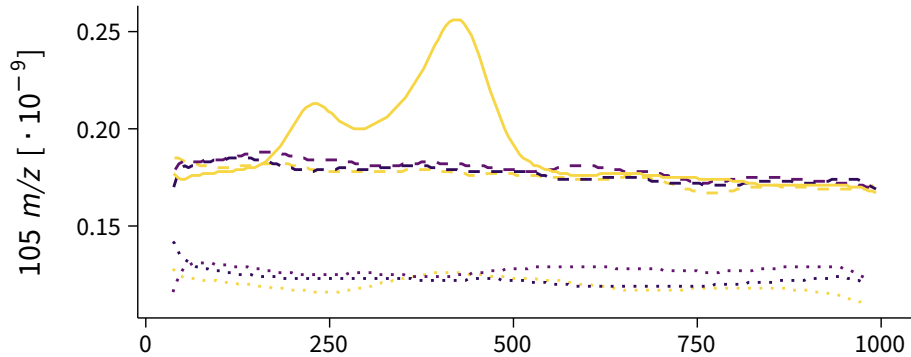
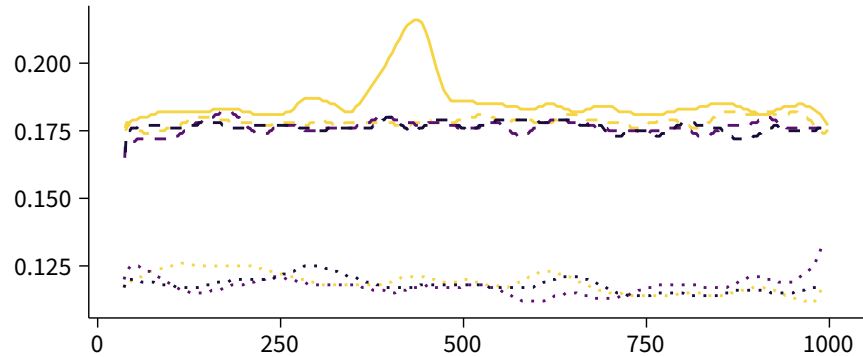



With internal standard**Without internal standard****PET content [mg g^{-1}]****Type**

···· Clean run after

-- Oxalate after

— Sample